

Innovative Use of Opsite Flexigrid™ for Digital Photography in Rhinoplasty

Denis Codazzi¹, Maria Alessandra Bocchiotti¹, Bernardo Righi², Enrico Robotti^{2*}

1. Department of Plastic Surgery, University of Turin, San Giovanni Battista Hospital, Turin, Italy;
2. Department of Plastic Surgery, Riuniti Hospital, Bergamo, Italy

Dear Editor

Standardization of photography in plastic surgery is fundamental for pre-operative surgical planning, comparative post-operative assessment, and demonstration of surgical results.¹ In rhinoplasty, slight changes in patient or camera position can lessen nasal hump, vary nose size, and alter skin tension.² In order to prevent these common errors, photographic standardization with high-quality equipment (camera, lens, and lighting), consistent room set up and systematic patient position are mandatory.²

The authoritative Institute of Medical Illustrators³ published its guidelines about “Rhinoplasty and Septorhinoplasty Photography”: One of the most important concerns is about the use of standard viewfinder alignment grids to help finding both horizontal (Frankfurt and Reid planes first) and vertical reference planes during shooting. However, some cameras lack this grid at all and some other have grid with only four axes leaving focus point without reference lines. (Figure 1)



Fig. 1: The commonest four axes grid leaves focus point without reference lines.

We thought about a new application of Opsite Flexigrid™ (Smith and Nephew Medical Limited, Hull, HU3 2BN, England) which is a transparent, adhesive film dressing, with a measurement grid (Figure 2).



Fig. 2: Opsite Flexigrid™ 10x12 Cm.

*Corresponding Author:

Enrico Robotti, MD,
Department of Plastic Surgery,
Riuniti Hospital,
Bergamo, Italy.

E-mail: bernardo.righi@libero.it

Received: June 9, 2012

Accepted: October 17, 2012

An Opsite Flexigrid rectangle is tailored with scissors on screen camera dimensions (Figure 3).

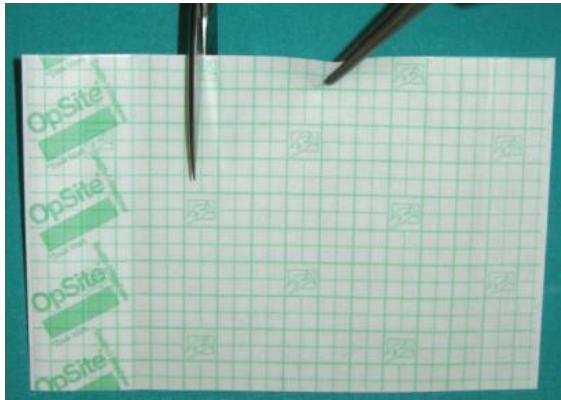


Fig. 3: Opsite Flexigrid™ is tailored with scissors on screen camera dimensions.

After removing the white back sheet (Figure 4), we turned on the camera and centered one of the grid intersections on camera viewfinder (Figure 5). The lines of the grid followed the main axes of the screen.

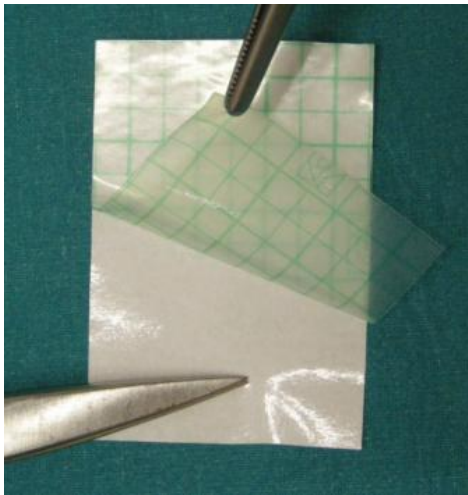


Fig. 4: White back sheet is removed.

The grid did not alter subject visibility and allowed the alignment of facial landmarks⁴ in all conventional rhinoplasty pictures. This is a cheap (0.82 euro for 6x7 Cm sample, 2.04 for 10x12 Cm sample), quick and reversible way to mechanically add to digital camera a frequent lacking display option.

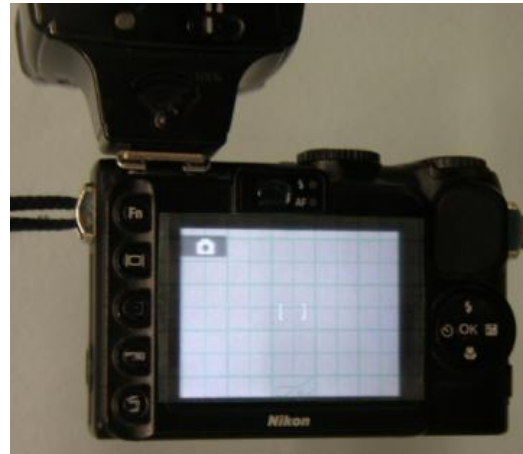


Fig. 5: Grid is positioned on camera screen.

CONFLICT OF INTEREST

The authors declare no conflict of interest.

KEYWORDS:

Opsite flexigrid; Digital Photography; Rhinoplasty

Please cite this paper as:

Codazzi D, Bocchiotti MA, Righi B, Robotti E. Innovative Use of Opsite Flexigrid™ for Digital Photography in Rhinoplasty. *World J Plast Surg* 2013;2(1): 50-51.

REFERENCES

- 1 Galdino GM, DaSilva And D, Gunter JP. Digital photography for rhinoplasty. *Plast Reconstr Surg* 2002;**109**:1421-34.
- 2 Archibald DJ, Carlson ML, Friedman O. Pitfalls of nonstandardized photography. *Facial Plast Surg Clin North Am* 2010;**18**:253-66.
- 3 Institute of Medical Illustrators, Great Britain. Rhinoplasty and septorhinoplasty photography. *J Vis Commun Med* 2007;**30**:135-9.
- 4 Ettorre G, Weber M, Schaaf H, Lowry JC, Mommaerts MY, Howaldt HP. Standards for digital photography in cranio-maxillofacial surgery-Part I: Basic views and guidelines. *J Craniomaxillofac Surg* 2006;**34**:65-73.